

TRIG

COMPONENT TESTER

HOLD OFF

SCIENTIFIC

1 2 5 10 20

V


AC

DC

FLJ0.2V

INTENS

FOCUS

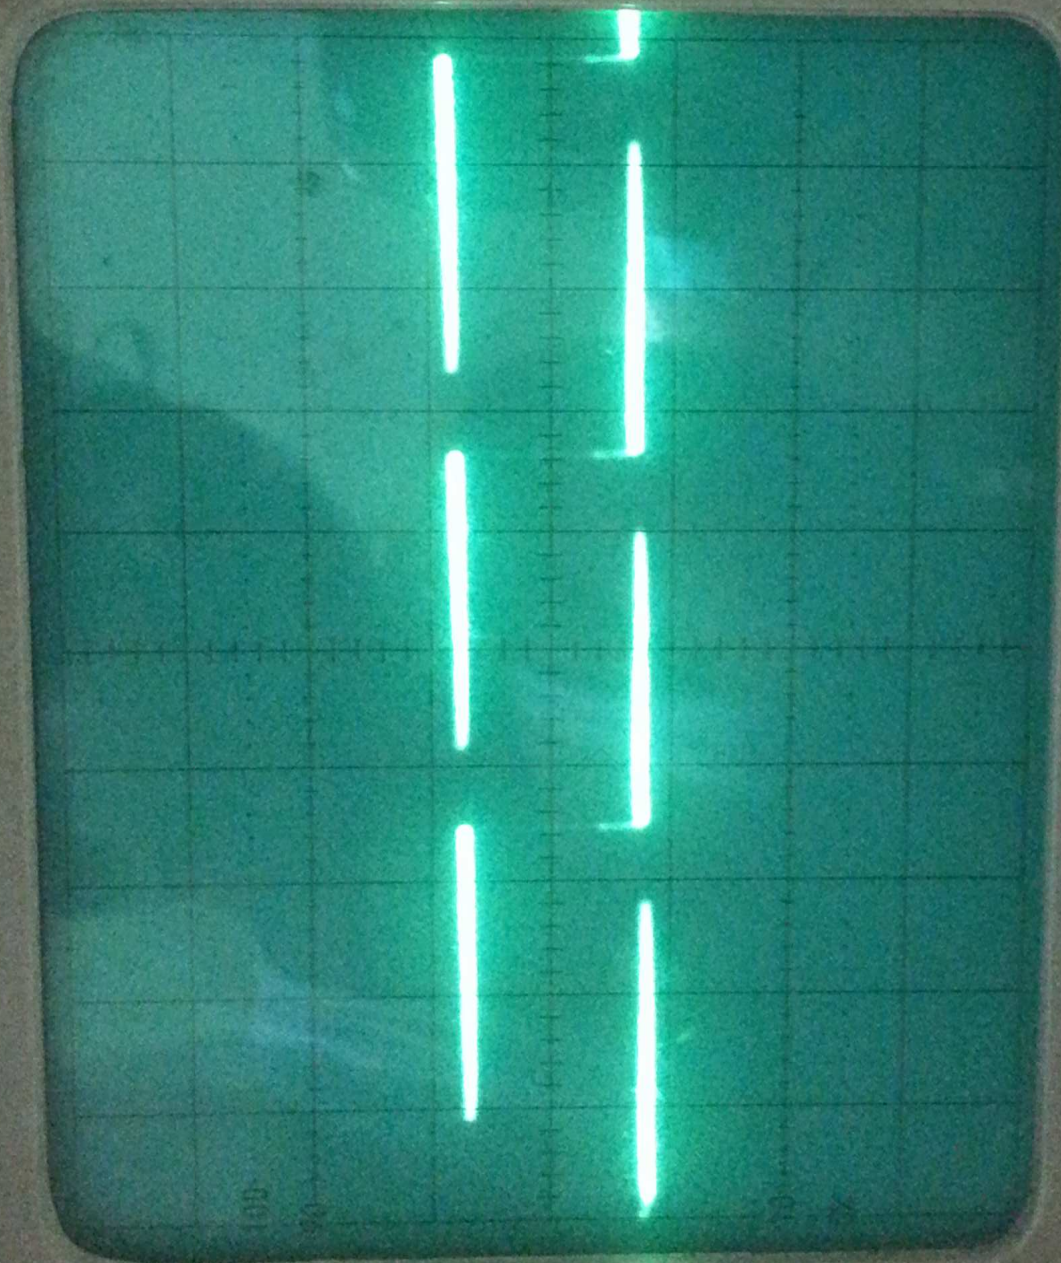

100

50

50

100

INTENS

FOCUS